

Embrace TALK Monitor


Embrace TALK Monitor

Setting Date and Time


Preparing Your Lancing Device

lancet.


Front of the Embrace TALK Monitor

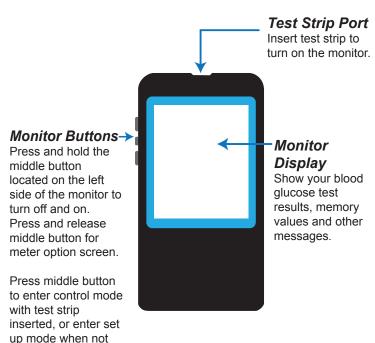

Back of the Embrace TALK Monitor

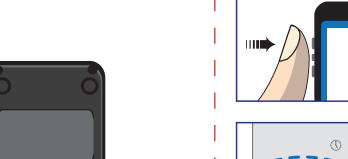


Press and hold the middle button to turn on the meter.



Current year will flash,

vour choice.




from the lancet. Place the lancing device cap back into the lancing device

1 Twist off the lancing device

cap and insert an unused

Twist the protective cover off




and adjust the puncture setting (1 is lightest and 5 is deepest).



4 Pull back on the lancing device



5 Press the button to lance.



Battery Compartment Holds two AAA batteries battery cover.






the arrow bottons, press the

center button in to confirm

Testing Your Blood Glucose



1 Insert the test strip to turn on the monitor.





3 Lance your finger.

Testing Your Blood Glucose



testing

4 Bring your lanced finger close to the tip of the test strip as shown. Blood will be pulled in when contact with the tip of the test strip is made.



5 Your blood glucose result will show up in six seconds.

Recalling Memory



1 Turn on the monitor by pressing and holding the center button in.

2 Press the center button in again to enter function mode. 3 Press the center button again when "mem"

icon flashes to enter memory recall. Press the top button to see stored results from the most

recent to oldest, Your monitor can hold up to 300 dates and time stamped results. Control solution results will be flagged by "ctl" icon at the lower left hand corner. When the meter memory is empty, the screen will show "nil".







Scroll down to see the average of results. The averages are 7, 14 and 30 days.







Problem Solving

Message Description and Remedy



Electronic malfunction. Take the batteries out and insert them into the monitor again and turn on. If the message is still there, contact 1-877-979-5454



Used test strip.

Insert a new unused test strip and test



Not enough blood in the test strip. Insert a new test strip and test again. Make sure the blood fills the confirmation window completely.

CAUTION: IF YOU SEE "HI" OR "LO" DISPLAYED, YOUR BLOOD GLUCOSE LEVEL MAY BE ABOVE 600 MG/DL OR BELOW 20 MG/DL, REPEAT TESTING. IF YOU STILL RECEIVE THE SAME RESULT. CALL YOUR PHYSICIAN OR

Problem Solving

Message Description and Remedy



Test result is higher than 600 mg/dL. Use a new test strip and test again. If the result is still the same, call your physician or healthcare professional immediately.



LO Test result is lower than 20 mg/dL. Use a new test strip and test again. If the result is still the same, call your physician or healthcare professional immediately.

Note: Please refer to the Embrace TALK instruction manual for more complete and detailed instructions and important safety warnings





Manufactured for: **OMNIS**[®]

> 1309 Elm Hill Pike Nashville, TN 37210 1-877-979-5454 www.EmbraceTalk.com

trademark of Omnis Health.



Please refer to the Embrace TALK instruction

∧ Note

manual for more complete and detailed instructions and important safety warnings.